



Room 105 update

Brachmann

Initial performance

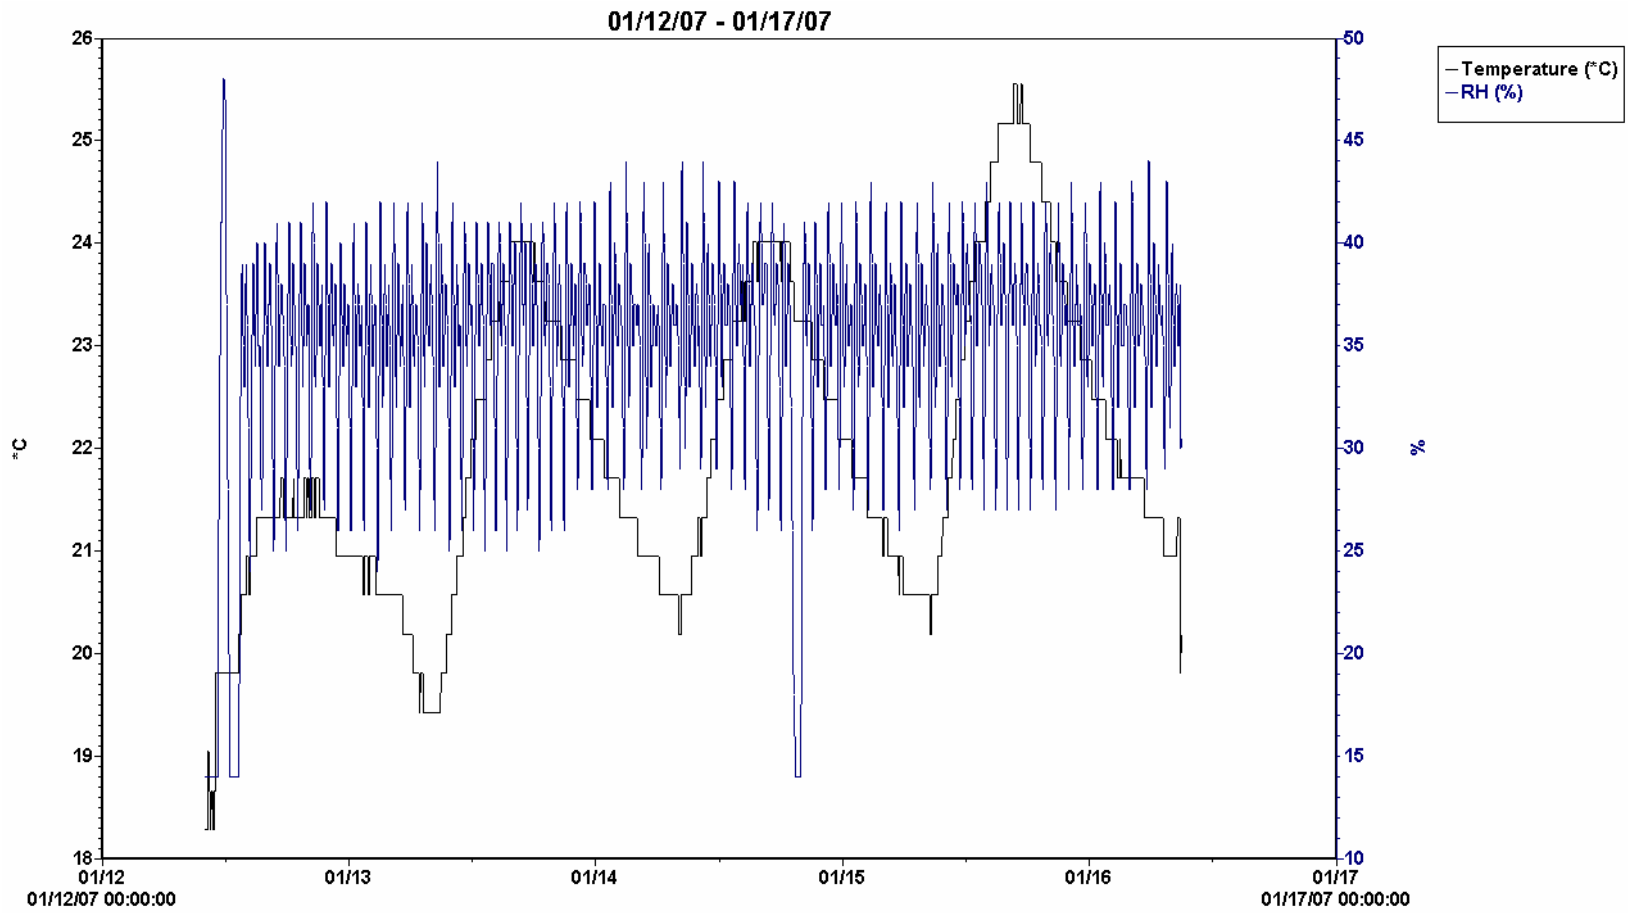

Adjusted performance

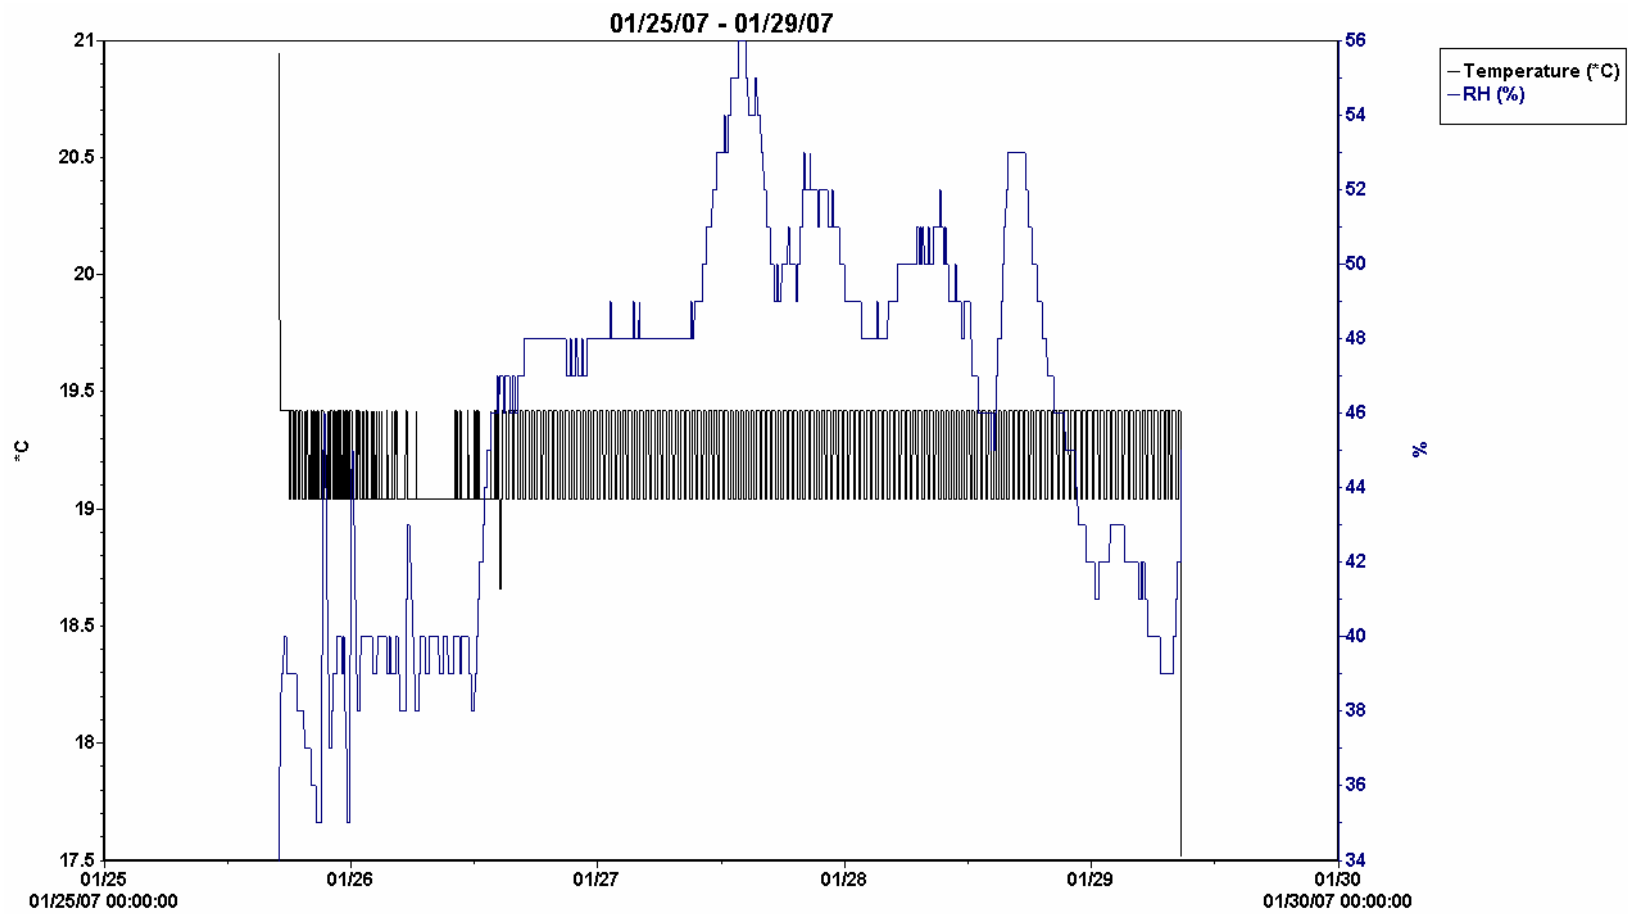

Next steps

- Tweak HVAC system to reduce RH swings
- Electrical work is done
- Access to HVAC control system is being granted by CEF group (not setup yet)
- After Beijing meeting
 - Test PPS system
 - Final approval of LSS system
 - Installation of Millenia (Pump) and Mira (oscillator)
 - Test 3 MHz Pockels cell